

Document made available under the Patent Cooperation Treaty (PCT)

International application number: PCT/GB05/000142

International filing date: 17 January 2005 (17.01.2005)

Document type: Certified copy of priority document

Document details: Country/Office: GB
Number: 0403968.1
Filing date: 24 February 2004 (24.02.2004)

Date of receipt at the International Bureau: 16 March 2005 (16.03.2005)

Remark: Priority document submitted or transmitted to the International Bureau in compliance with Rule 17.1(a) or (b)



World Intellectual Property Organization (WIPO) - Geneva, Switzerland
Organisation Mondiale de la Propriété Intellectuelle (OMPI) - Genève, Suisse



Port/GB2005/000142



INVESTOR IN PEOPLE


The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

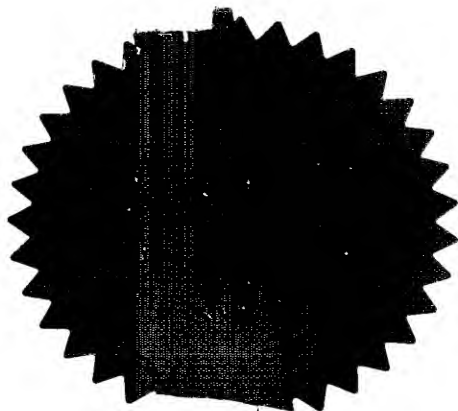

Signed *AmBrewer.*

Dated 4 March 2005




Handwritten text, possibly a signature or date, located near the bottom center of the page.



24FEB04 EB75497-1 002832
P01/7700-0-00-0403968.1 CHEQUE

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

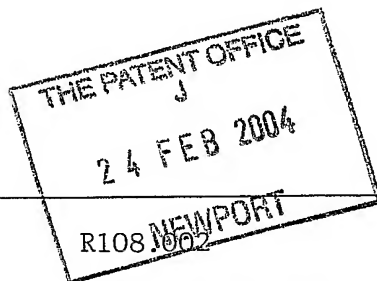

The Patent Office

Cardiff Road
Newport
South Wales
NP10 8QQ

1. Your reference

2. Patent application number

(The Patent Office will fill in this part)

0403968.1

24 FEB 2004

3. Full name, address and postcode of the or of each applicant (*underline all surnames*)

Rescu-Bed Limited
25 Park Drive
Leicester Forest East
Leicester
LE3 3FG

Patents ADP number (*if you know it*)

If the applicant is a corporate body, give the country/state of its incorporation

8735540001
United Kingdom

4. Title of the invention

Emergency evacuation apparatus for a bed-ridden person

5. Name of your agent (*if you have one*)

SERJEANTS

"Address for service" in the United Kingdom to which all correspondence should be sent (*including the postcode*)

25 The Crescent
King Street
Leicester
LE1 6RX

Patents ADP number (*if you know it*)

1461001 /

6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (*if you know it*) the or each application number

Country

Priority application number
(*if you know it*)

Date of filing
(*day / month / year*)

7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application

Number of earlier application

Date of filing
(*day / month / year*)

8. Is a statement of inventorship and of right to grant of a patent required in support of this request? (*Answer 'Yes' if:*

Yes

- a) any applicant named in part 3 is not an inventor, or
 - b) there is an inventor who is not named as an applicant, or
 - c) any named applicant is a corporate body.
- See note (d))

Patents Form 1/77

9. Enter the number of sheets for any of the following items you are filing with this form.
Do not count copies of the same document

Continuation sheets of this form

Description 9

Claim(s) 3

Abstract 1

Drawing(s) 5

10. If you are also filing any of the following, state how many against each item.

Priority documents

Translations of priority documents

Statement of inventorship and right to grant of a patent (*Patents Form 7/77*) 1

Request for preliminary examination and search (*Patents Form 9/77*) 1

Request for substantive examination (*Patents Form 10/77*) 1

Any other documents
(please specify)

11. I/We request the grant of a patent on the basis of this application.

Signature

Serjeants

Date

SERJEANTS

23 February 2004

12. Name and daytime telephone number of person to contact in the United Kingdom
Darran Thacker
0116 233 2626

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 08459 500505.
- Write your answers in capital letters using black ink or you may type them.
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- Once you have filled in the form you must remember to sign and date it.
- For details of the fee and ways to pay please contact the Patent Office.

TITLE

Emergency evacuation apparatus for a bed-ridden person

DESCRIPTION

5 Technical Field

The invention relates to an improved evacuation apparatus to enable the rapid and safe removal of bedridden people from hospitals, old persons homes and other buildings in emergency situations.

10 Background Art

In the event of an emergency requiring the fastest possible evacuation, it is a major concern that the most vulnerable people present the greatest difficulty in being evacuated to safety. The old and infirm, and bed-ridden hospital patients, being persons with limited mobility, are dependent upon helpers to execute their safe evacuation.

British Patent Application 2324738 describes an apparatus that can be used to evacuate a bed-ridden person from a bed in an emergency situation. The apparatus comprises a rigid tray of a length substantially equal to that of the mattress on which the person to be evacuated is lying. Wheels, glide members, roller balls or castors are mounted on the base tray to facilitate its movement over the floor and straps are secured to the tray for wrapping around the mattress to thereby restrain and cocoon the person. Lifting handles may be provided so that the person can be lifted down from the bed and placed on the floor or evacuated out of the building.

25 Australian Patent 667183 describes a disposable stretcher fabricated from a folded board material that provides a substantially flat base on which a person can lie. The base has a single transverse fold line to enable it to be folded for storage purposes. Two longitudinal fold lines allow edge parts of the base to be folded upwardly to form walls that provide longitudinal reinforcement to the base. A number of hand holes are provided around the periphery of the base and can receive straps to secure the person to the stretcher.

Many hospitals and care homes for the old and infirm are gradually replacing traditional beds of fixed construction with modern adjustable beds. These can be electrically or manually operated to adjust the profile of the mattress to provide better ergonomic support for the person lying on the bed. A conventional adjustable bed has four panels positioned underneath the mattress that can bend relative to each other. The two panels closest to the foot of the bed support the legs of the person and can bend to form a knee-break. The panel closest to the head of the bed can be raised or lowered to help the person to sit up and provides a backrest. The remaining panel does not normally move and supports the hips and waist of the person.

The apparatus described in British Patent Application 2324738 can only be used with traditional beds of fixed construction. There is therefore a need for an emergency evacuation apparatus that is suitable for use with a modern adjustable bed.

Summary of the Invention

The invention provides an emergency evacuation apparatus for removing a bed-ridden person from a bed in an emergency situation, comprising a base tray having at least one transverse fold line to allow the base tray to bend as two or more panels; and mechanical locking means operable between an unlocked condition in which the base tray is able to bend along the transverse fold line and a locked condition in which the base tray is unable to bend along the transverse fold line and to provide the base tray with sufficient longitudinal rigidity to support the weight of an adult person.

In normal use, the base tray is placed between the panels of an adjustable bed and the mattress. The number and position of transverse fold lines will be selected so that the base tray has the same number of panels as the bed. For example, if the adjustable bed has four panels then the base tray will be provided with three transverse fold lines so that the base tray can bend as four panels. The base tray will bend in register with the associated underlying panels of the adjustable bed but does not hinder the operation of the bed in any way. Preferably, the base tray has substantially the same width as the bed from which the person is to be evacuated.

It is normally preferred that the mechanical locking means are operable in an emergency situation to lock the panels of the base tray in a co-planar configuration so that the bed-ridden person can be removed in a prone position. However, it is also possible that the mechanical locking means are operable to lock the panels of the base tray at any predetermined angle to each other. For example, if the base tray has four panels then the three panels closest to the foot end of the emergency evacuation apparatus can be locked in a co-planar configuration but the fourth panel at the head end can be locked at a slight angle with respect to the plane of the remainder of the base tray to provide additional support by raising the person's back.

10

It will be readily appreciated that the mechanical locking means must be strong enough to provide the base tray with sufficient longitudinal rigidity to allow the emergency evacuation apparatus to support the weight of an adult person.

15

The mechanical locking means can be of any suitable construction or type. For example, a rigid locking bolt can be made to slide across the transverse fold line when the panels are co-planar. The locking bolt is preferably secured to the underside of one of the panels and can be received in an associated locking aperture provided on the underside of the other panel to prevent the base tray from bending along the transverse fold line. The locking bolt can also be slidably received in a pair of channels or sleeves on the underside of the base tray that extend on both sides of the transverse fold line.

20

A plurality of mechanical locking means can be provided for each transverse fold line.

25

The mechanical locking means can be operated independently of each other or together in a single locking action

30

If the base tray has more than one transverse fold line then separate mechanical locking means can be provided for each transverse fold line so that respective pairs of panels can be selectively locked together. Alternatively, a single mechanical locking means is provided. For example, a locking bolt can be slidably received in channels or sleeves on the underside of the base tray that extend on both sides of each

transverse fold line. The locking bolt has a number of pivot regions that are aligned with the transverse fold lines when the locking bolt is in the unlocked condition. In an emergency situation, the locking bolt can be made to slide when the panels are coplanar so that the pivot regions are no longer aligned with the transverse fold lines and rigid parts of the locking bolt next to the pivot regions extend across the transverse fold lines. If the pivot regions only allow the locking bolt to bend in one plane then the panels can be locking in position by rotating the locking bolt through 90°, for example.

To facilitate its movement over the floor, the underside of the base tray is preferably provided with wheels, glide members, roller balls or castors. These can be fitted in channels provided on the underside of the base tray.

A number of u-shaped runners can be fixed to the underside of the base tray to improve the strength and rigidity of the two or more panels. The runners preferably extend longitudinally to define a pair of parallel channels into which the wheels, glide members, roller balls or castors can be fitted. The runners do not extend across the at least one transverse fold line and their ends can be cut away or profiled so that they do not prevent the panels of the base tray from bending relative to each other. Strips of high-density foam can be fixed to the underside of the base tray along its edges and between the runners to help support the base tray on top of the panels of the adjustable bed.

The wheels, glide members, roller balls or casters can be retractable so that they only project beyond the underside of the base tray or the channels when they are needed in an emergency situation. Alternatively, the wheels, glide members, roller balls or castors can be received in recesses or channels provided in the top surface of the panels of the adjustable bed.

The base tray can further include a pair of longitudinal fold lines to allow the sides of the base tray to be inclined slightly. The applicant has found that this does not significantly increase the longitudinal rigidity of the emergency evacuation apparatus

but does prevent the sides of the base tray from impeding its movement along the floor. The longitudinal fold lines define a central panel for supporting the person and two side panels.

- 5 Straps can be secured to the base tray for wrapping around the person in an emergency situation. The straps are preferably provided with snap-fit couplings which permit them to be connected together to encircle the mattress and person prior to tightening them to draw the mattress around the person. Mechanical tensioning means may be provided.

10

- Many adjustable beds have inbuilt hydraulic raising and lowering devices, and a removable tail-board or frame. To evacuate a person in an emergency situation, first of all the adjustable bed is electrically or manually operated so that the panels of the base tray lie in the same plane or at a predetermined angle to each other. The straps
15 are then tightened around the person to secure the person on the base tray. If the panels are co-planar then this tightening of the straps also causes the base tray to bend slightly along the longitudinal fold lines. The mechanical locking means are operated from the unlocked condition to the locked condition to maintain the panels in the desired configuration (normally co-planar) and provide the base tray with sufficient
20 longitudinal rigidity to support the weight of an adult person. It will be appreciated that operating the mechanical locking means immediately forms an extremely robust and rigid structure that is capable of being used as a stretcher to evacuate the person to safety.

- 25 After tightening the straps around the mattress and person to cocoon and restrain the person, the adjustable bed is lowered to its minimum height, the tail-board or frame removed and the rigid base tray pulled down the bed to an intermediate position in which it tips with its foot end resting on the floor and its head end resting on the foot end of the bed. The base tray can then be gently lowered on to the floor.

30

If the tail-board or frame of the adjustable bed is not removable then it can include rollers or fixed projections for engagement with the runners fixed to the underside of

the base tray. In this case, the foot end of the rigid base tray is raised and then pulled over the tail-board or frame with the rollers or fixed projections engaging with the runners to act as guides and prevent the base tray deviating from side to side. The base tray is placed in an intermediate position in which it tips with its foot end resting on the floor and its head end resting on the tail-board or frame. The head end can then be gently lowered to the floor.

The base tray can be made of polypropylene so that it is strong and lightweight. If u-shaped runners are provided then these can be made of aluminium and riveted to the underside of the base tray.

The base tray is preferably formed in a single piece with the transverse and longitudinal fold lines being hydraulically pressed into the base tray.

To facilitate the subsequent evacuation of the person, carrying handles can be secured to the sides of the base tray. A handle can also be secured to one end of the base tray to assist in raising the base tray or pulling it down the bed to the intermediate position.

Although the emergency evacuation apparatus is intended to be used primarily on adjustable beds, it will be appreciated that it can also be used on traditional beds of fixed construction.

Drawings

Figure 1 is a side view of an adjustable bed;

Figure 2 is a top view of an emergency evacuation apparatus in accordance with the present invention;

Figure 3 is a bottom view of the apparatus of Figure 2 with the locking bolts in an unlocked condition;

Figure 4 is a cross-section view taken along line AA shown in Figure 3 with the locking bolts in an unlocked condition;

Figure 5 is a cross-section view taken along line AA shown in Figure 3 with the locking bolts in a locked condition;

Figure 6 is an end view of the apparatus of Figure 2;

Figure 7 is a side view showing the apparatus of Figure 2 placed on an adjustable bed;

Figure 8 is an end view showing the apparatus of Figure 2 being used to restrain a person; and

5 Figure 9 is an end view showing the apparatus of Figure 2 being raised over the tail-board of an adjustable bed.

Figure 1 shows an adjustable bed having four panels 2 supporting a mattress 3. The foot end and head end of the bed are provided with fixed tail-boards 4 to prevent the
10 mattress 3 from sliding off the panels 2. The panels can be electrically or manually operated to adjust the profile of the mattress 3 to support the person P in a number of different ways. The panel 2a closest to the head end of the bed acts as a backrest and can be raised or lowered to help the person P sit up or lie down. The intermediate panel 2b does not move and supports the hips and waist of the person P. The two
15 panels 2c and 2d closest to the foot end of the bed can bend together to form a knee-break.

With reference to Figures 2 to 6, an emergency evacuation apparatus 10 has a base tray 11 formed from a single sheet of polypropylene. Three transverse fold lines 12a,
20 12b and 12c are hydraulically pressed into the polypropylene sheet to divide the base tray 11 into four panels 13a to 13d. The base tray 11 has substantially the same width as the panels 2 of the adjustable bed. Moreover, the transverse fold lines 12 are positioned so that the four panels 13 of the base tray 11 are substantially the same size as the associated panels 2 of the adjustable bed.

25 Two longitudinal fold lines 14a and 14b are hydraulically pressed into the polypropylene sheet to divide the base tray 11 into a central panel 15a and two side panels 15b.

30 A number of u-shaped aluminium runners 16 are riveted to the underside of the central panel 15a of the base tray 11 to define a pair of parallel channels. As best shown in Figure 4, the runners 16 do not extend across the transverse fold lines 12

and their facing ends are cut away or profiled so that they do not prevent the panels 13 bending relative to each other. A pair of wheels 17 is provided in the channels at each end of the base tray.

5 Two strips 18 of high-density foam having substantially the same depth as the runners 16 are attached to the underside of the side panels 15b of the base tray 11 and help support the base tray on top of the panels 2 of the adjustable bed. The strips of high-density foam can be replaced by u-shaped aluminium runners to provide additional strength and rigidity to the side panels 15b. A further strip 19 of high-density foam is
10 attached to the underside of the central panel 15a of the base tray 11. The strips 18 and 19 of high-density foam are cut into sections so that they do not extend across the transverse fold lines 12.

15 In normal use, the part of each wheel 17 that projects outside the associated runner 16 is received in a recess (not shown) provided in the top surface of the panels 2a and 2d of the adjustable bed.

20 Six rigid locking bolts 20 are received in the u-shaped runners 16 and retained by inwardly extending lips (not shown). In Figures 3 and 4 the locking bolts 20 are in an unlocked condition and do not extend across the transverse fold lines 12a, 12b and 12c so the panels 13a to 13d of the base tray 11 are free to bend relative to each other. In an emergency situation, the locking bolts 20 are moved to a locked condition by sliding them along the u-shaped runners 16 until they extend across the transverse fold lines 12a, 12b and 12c. This action locks the panels 13a to 13d together so that
25 the base tray 11 is made sufficiently rigid in the longitudinal direction to support the weight of an adult person.

30 Figure 7 shows how the base tray 11 is positioned on the adjustable bed such that the panels 13a to 13d are in register with the associated panels 2a to 2d. (It will be readily appreciated that the wheels 17 and the strips 18 of high-density foam have been omitted from Figure 6 to improve the clarity of the drawing.)

With reference to Figures 8 and 9, in an emergency situation, the adjustable bed is operated so that the panels 2 are lowered until they are horizontal and the panels 13 of the base tray 11 lie in the same plane. Straps 21 secured to the side of the base tray (not shown in Figures 2 to 6 to improve the clarity of those drawings) are tightened
5 around the person P to bend the base tray 11 along the longitudinal fold lines 14a and 14b and wrap the mattress 3 around the person to form a shielding cocoon of mattress material. (In practice, the applicant has found that the base tray 11 does not bend very much along the longitudinal fold lines 14a and 14b because of the thickness of the mattress. The angle of the side panels 15b relative to the central panel 15a has been
10 exaggerated to improve the clarity of the drawings.) Finally, the locking bolts 20 are operated from the unlocked condition to the locked condition as described above.

The adjustable bed is lowered to its minimum height and the rigid base tray 11 is raised and pulled over the fixed tail-board 4 at the foot end of the bed. The tail-board
15 4 is provided with a pair of rollers 5 which engage with the runners 16 to act as guides to prevent the base tray 11 deviating from side to side. The base tray 11 is placed in an intermediate position in which it tips with its foot end resting on the floor and its head end resting on the tail-board 4. The head end is gently lowered to the floor and the base tray 11.

20 The base tray 11 can be moved over the floor using the wheels 17. Carrying handles (not shown) secured to the sides of the base tray 11 can also be used to carry the base tray if the person has to be evacuated to safety.

25

CLAIMS

1. An emergency evacuation apparatus for removing a bed-ridden person from a bed in an emergency situation, comprising a base tray having at least one transverse fold line to allow the base tray to bend as two or more panels; and mechanical locking
5 means operable between an unlocked condition in which the base tray is able to bend along the transverse fold line and a locked condition in which the base tray is unable to bend along the transverse fold line and to provide the base tray with sufficient longitudinal rigidity to support the weight of an adult person.
- 10 2. An emergency evacuation apparatus according to claim 1, wherein the mechanical locking means is one or more rigid locking bolts.
3. An emergency evacuation apparatus according to claim 1 or claim 2, wherein
15 the base tray has three transverse fold lines to allow the base tray to bend as four panels.
4. An emergency evacuation apparatus according to any preceding claim,
20 wherein the underside of the base tray is provided with wheels, glide members, roller balls or castors to facilitate its movement over the floor.
5. An emergency evacuation apparatus according to claim 4, wherein the wheels,
glide members, roller balls or castors are fitted in channels on the underside of the base tray.
- 25 6. An emergency evacuation apparatus according to claim 4 or claim 5, further comprising u-shaped runners fixed to the underside of the base tray into which the wheels, glide members, roller balls or castors are fitted.
- 30 7. An emergency evacuation apparatus according to any preceding claim, further comprising straps secured to the base tray for wrapping around the person in an emergency situation to restrain the person.

8. An emergency evacuation apparatus according to claim 7, wherein the straps are provided with snap-fit couplings which permit them to be connected together to encircle the person prior to tightening them.

5 9. An emergency evacuation apparatus according to claim 7 or claim 8, wherein the base tray has two longitudinal folds lines defining a central panel for supporting the person and two side panels that can be bent out of the plane of the central panel by the straps.

10 10. An emergency evacuation apparatus according to any preceding claim, wherein the base tray is made of polypropylene.

11. An emergency evacuation apparatus according to any preceding claim, wherein the transverse and longitudinal fold lines are hydraulically pressed into the
15 base tray.

12. An emergency evacuation apparatus according to any preceding claim, further comprising carrying handles secured to the sides of the base tray.

20 13. An emergency evacuation apparatus according to any preceding claim, further comprising one or more strips of foam fixed to the underside of the base tray.

14. A combination of a bed and an emergency evacuation apparatus according to any preceding claim, wherein the base tray has substantially the same width as the
25 bed.

15. A combination of a bed and an emergency evacuation apparatus according to claim 6, wherein a tail-board of the bed includes rollers or fixed projections for engagement with the runners fixed to the underside of the base tray to assist the
30 removal of the apparatus from the bed.

14. An emergency evacuation apparatus substantially as described herein and with reference to the drawings.

TITLE

Emergency evacuation apparatus for a bed-ridden person

(Figure 2)

5

ABSTRACT

The invention provides an emergency evacuation apparatus for removing a bed-ridden person from a bed in an emergency situation. The apparatus includes a base tray 11 having at least one transverse fold line 12 to allow the base tray to bend as two or
10 more panels 13. This apparatus is therefore suitable for use with a modern adjustable bed which can be electrically or manually operated to adjust the profile of the mattress to provide better ergonomic support for the person lying on the bed. The base tray 11 also has mechanical locking means 20 operable between an unlocked condition where the base tray 11 can bend along the transverse fold line 12 and a locked condition
15 where the base tray 11 is unable to bend along the transverse fold line. The mechanical locking means 20 also provides the base tray 11 with sufficient longitudinal rigidity to support the weight of an adult person.



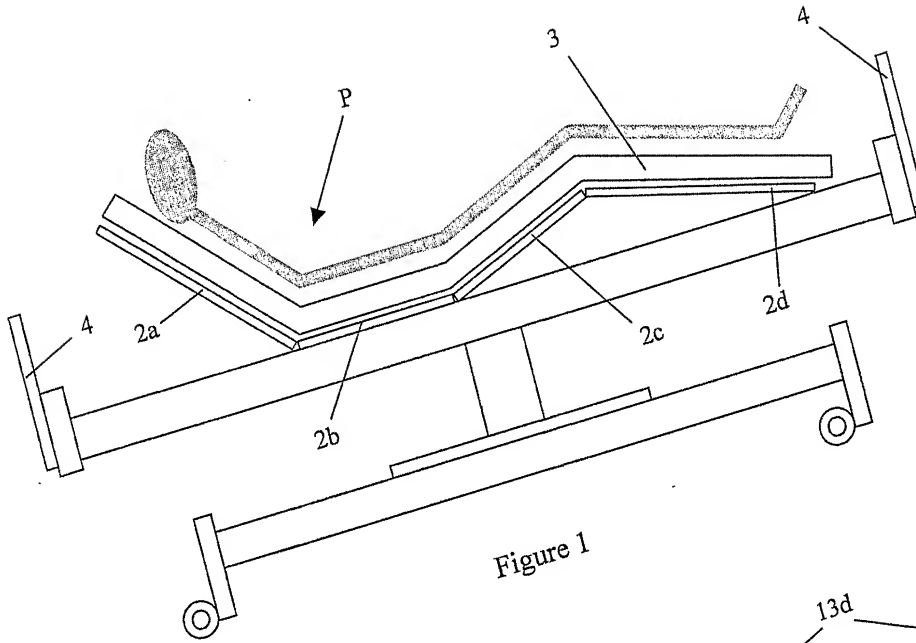


Figure 1

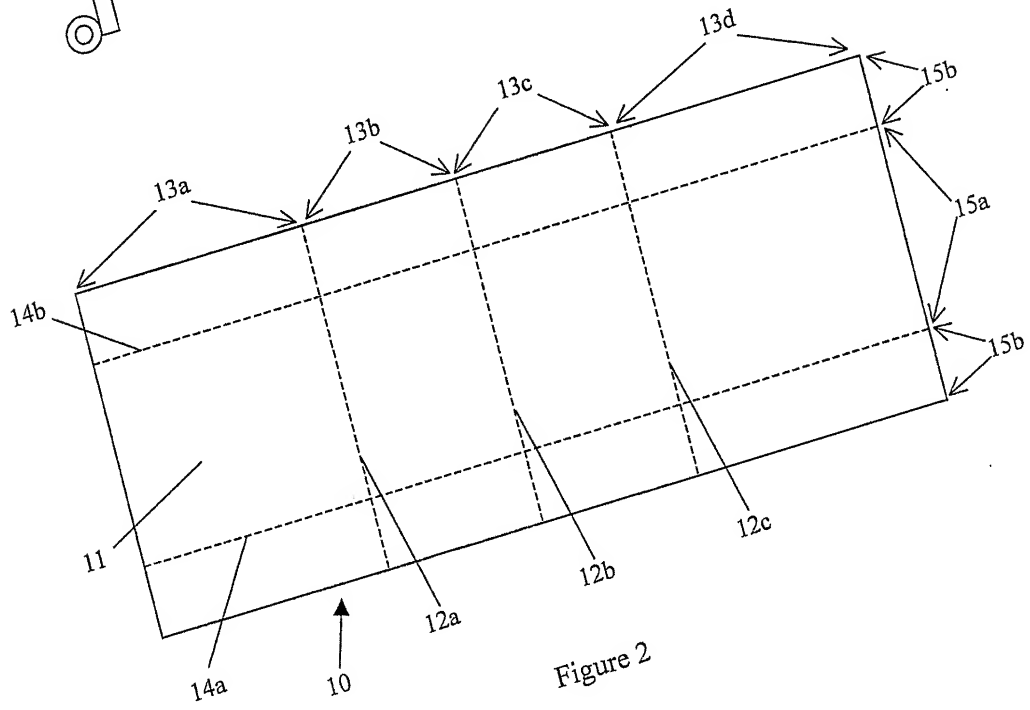


Figure 2



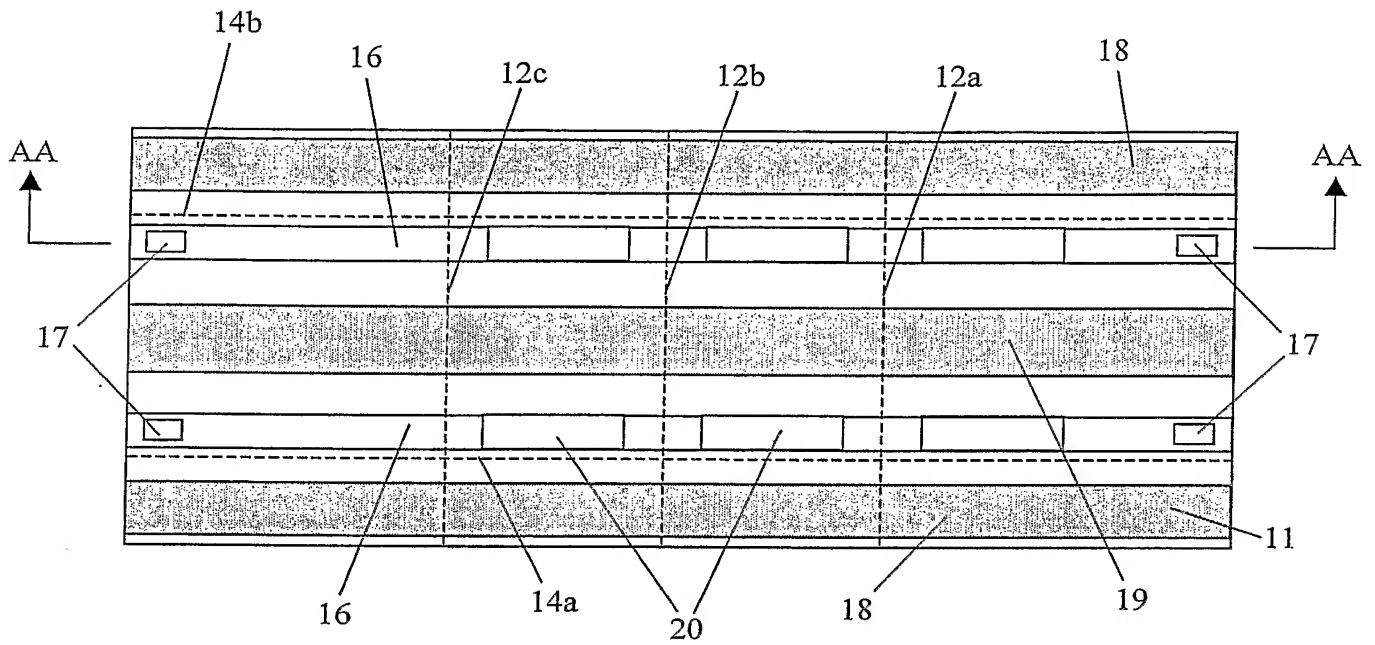


Figure 3

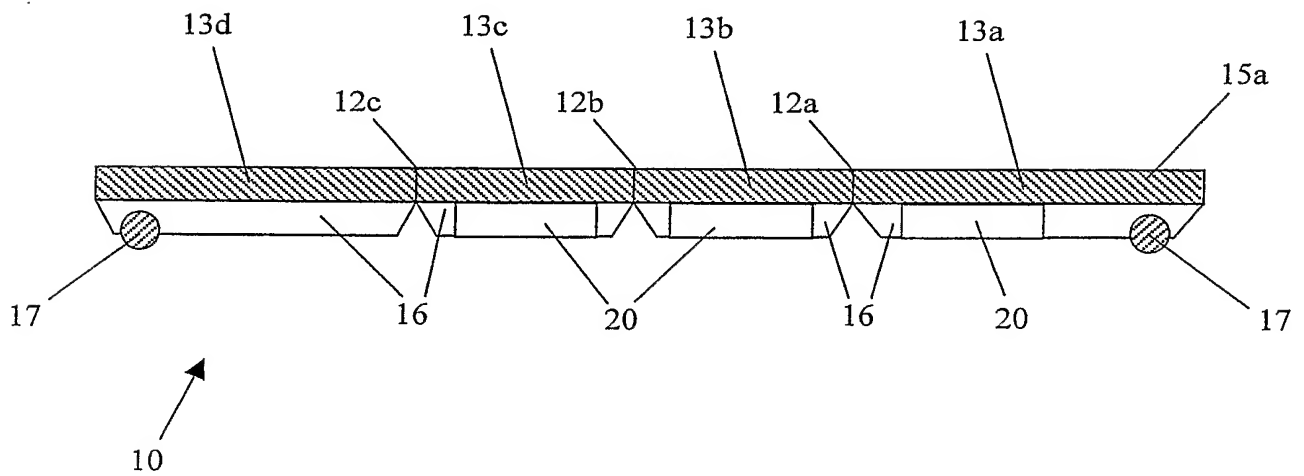


Figure 4



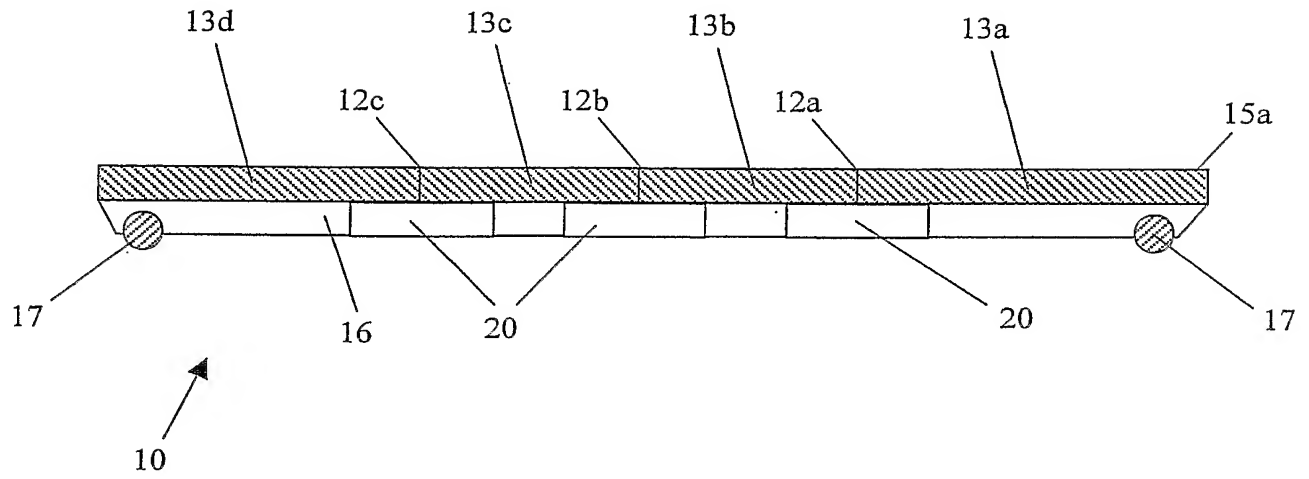


Figure 5

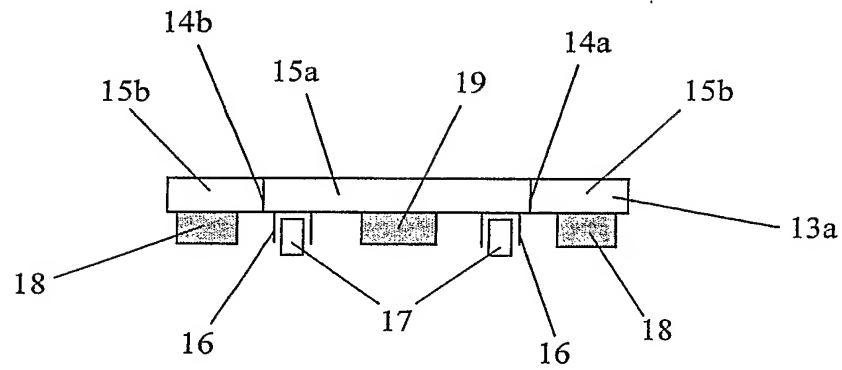


Figure 6



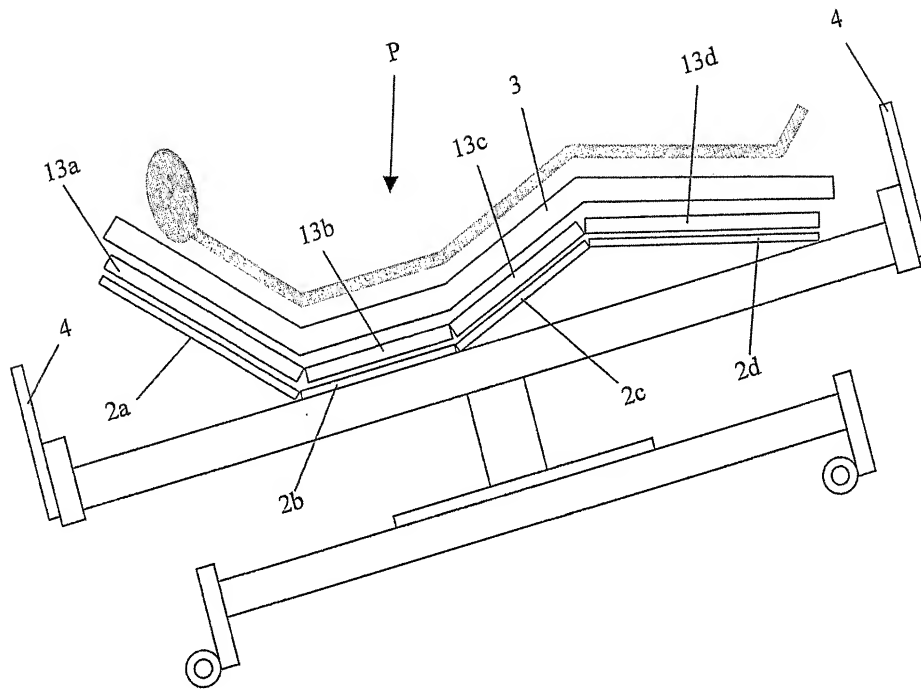


Figure 7



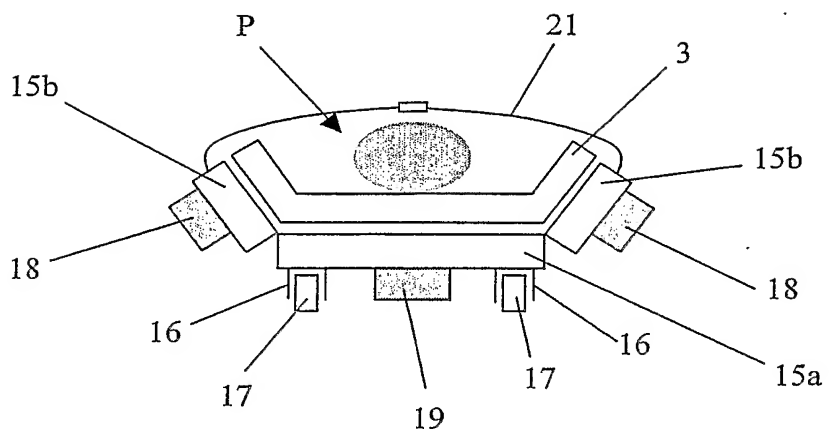


Figure 8

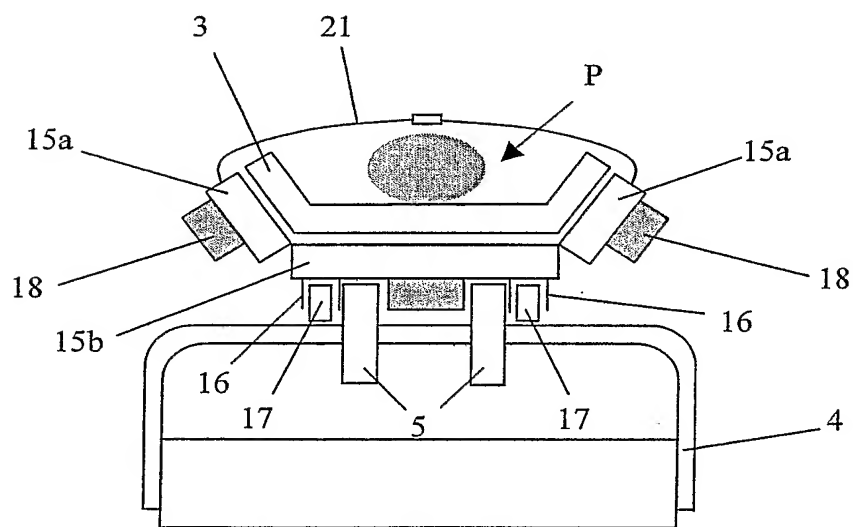


Figure 9

